RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

DrägerService®

Dräger

PMS Parts Reference Guide

Part Number: SP00216
Rev: -
Date: 31 May 2001
© 2001 Draeger Medical, Inc.

Microvent/Oxylog 2000

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

PMS Parts Reference Guide

This document is intended as a reference guide to assist in the replacement of routine maintenance parts.

Microvent / Oxylog 2000

Description	Part Number	Comments
		Microvent/Oxylog
12 month	4114768	
	R26807	O-Ring - 1x / 3x
	8410653	Diaphragm - 1x / 1x
	8400827	O-Ring - 2x / none
24 month	4114769	
	2M01524	Packing Ring - 1x / 2x
	D15330	O-Ring - 2x / 2x
	M16143	Washer - none / 2x
	8411599	Battery Pack - 1x / 1x
	D02316	Filter - 1x / 1x
	R24718	O-Ring - none / 1x
	2M12839	O-Ring - 1x / 1x
	R18566	O-Ring - 2x / none
72 month	*No kit*	
	8402745	Regulator - 1x / 1x
	Or 8411142	Reg Repair Set (Lorch)
	Or 8406678	Reg Repair Set (Knocks)

PMS Parts Reference Guide (continued)

Microvent Expiration Valve

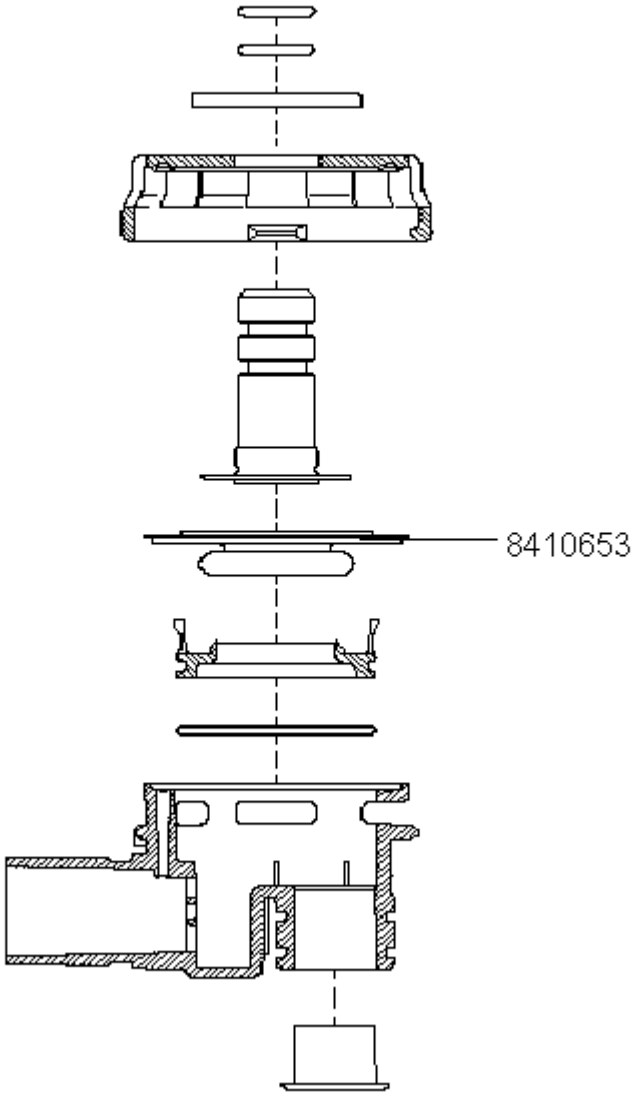

PMS Parts Reference Guide (continued)

Oxylog 2000 Respiration Valve

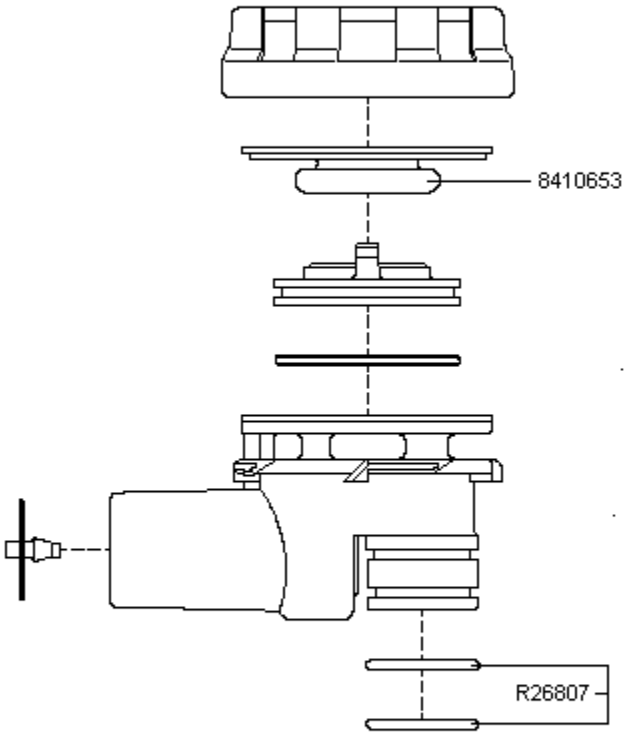

PMS Parts Reference Guide (continued)

Microvent / Oxylog 2000
Flow Sensor

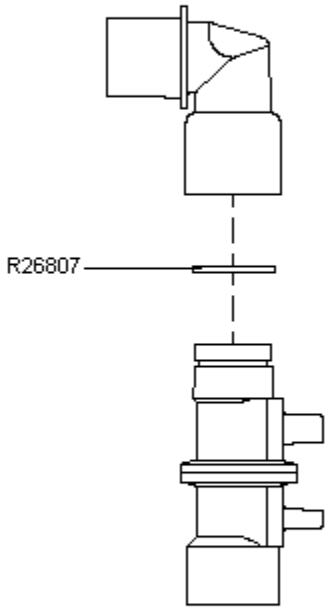

PMS Parts Reference Guide (continued)

Microvent

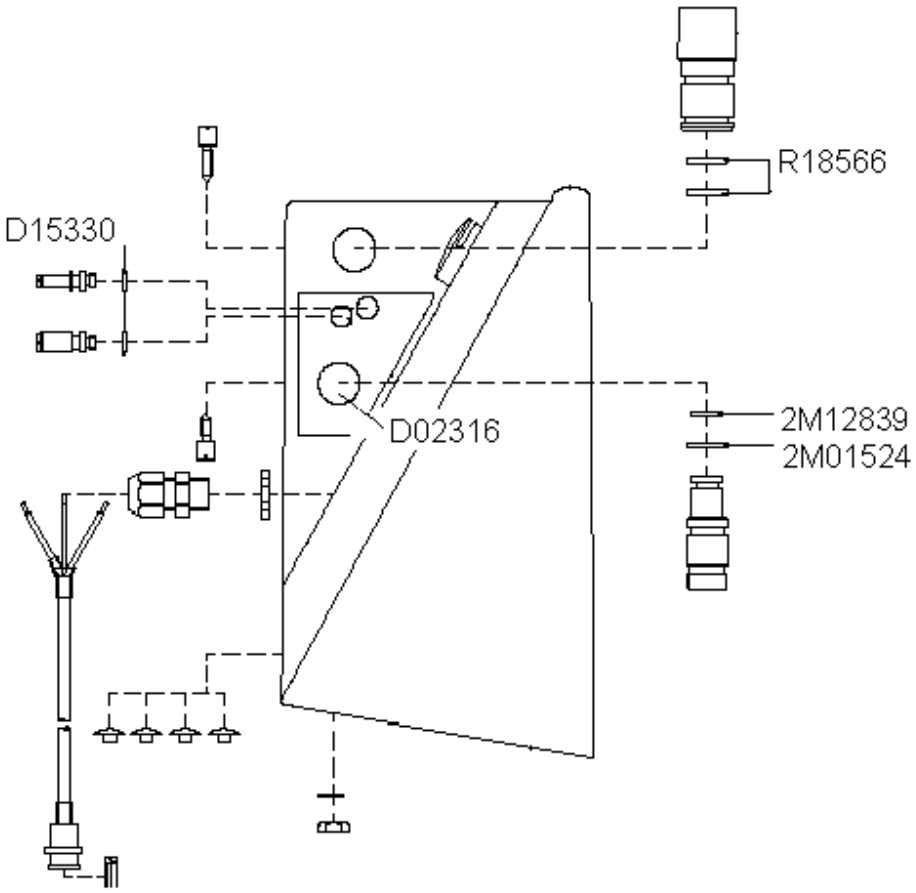

PMS Parts Reference Guide (continued)

Oxylog 2000

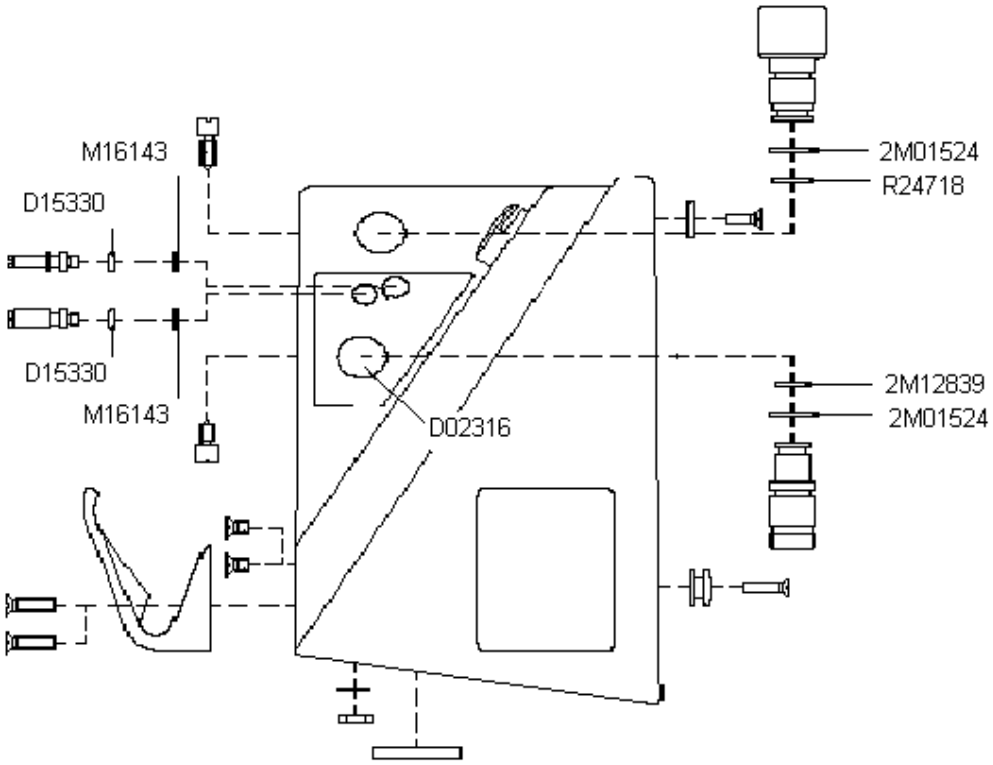

PMS Parts Reference Guide (continued)

Microvent / Oxylog 2000

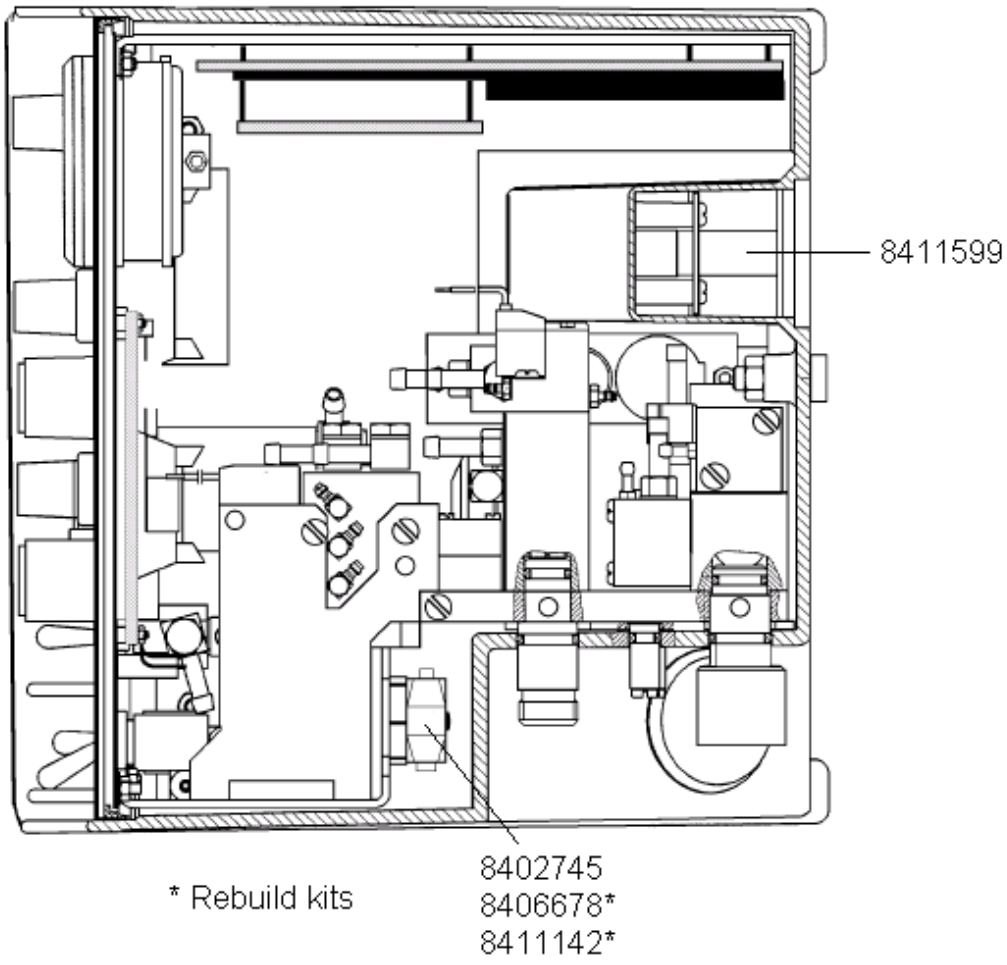

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

RETURN TO SERVICE PROCEDURE TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

DrägerService®

Dräger

DrägerService is a division of
Draeger Medical, Inc.
3122 Commerce Drive
Telford, PA 18969
Tel: (215) 721-5402
(800) 543-5047
Fax: (215) 721-5784
Web: www.draegermedical.com
Printed in the U.S.A.